

Agilent 16517A/16518A 1 GHz State / 4 GHz Timing

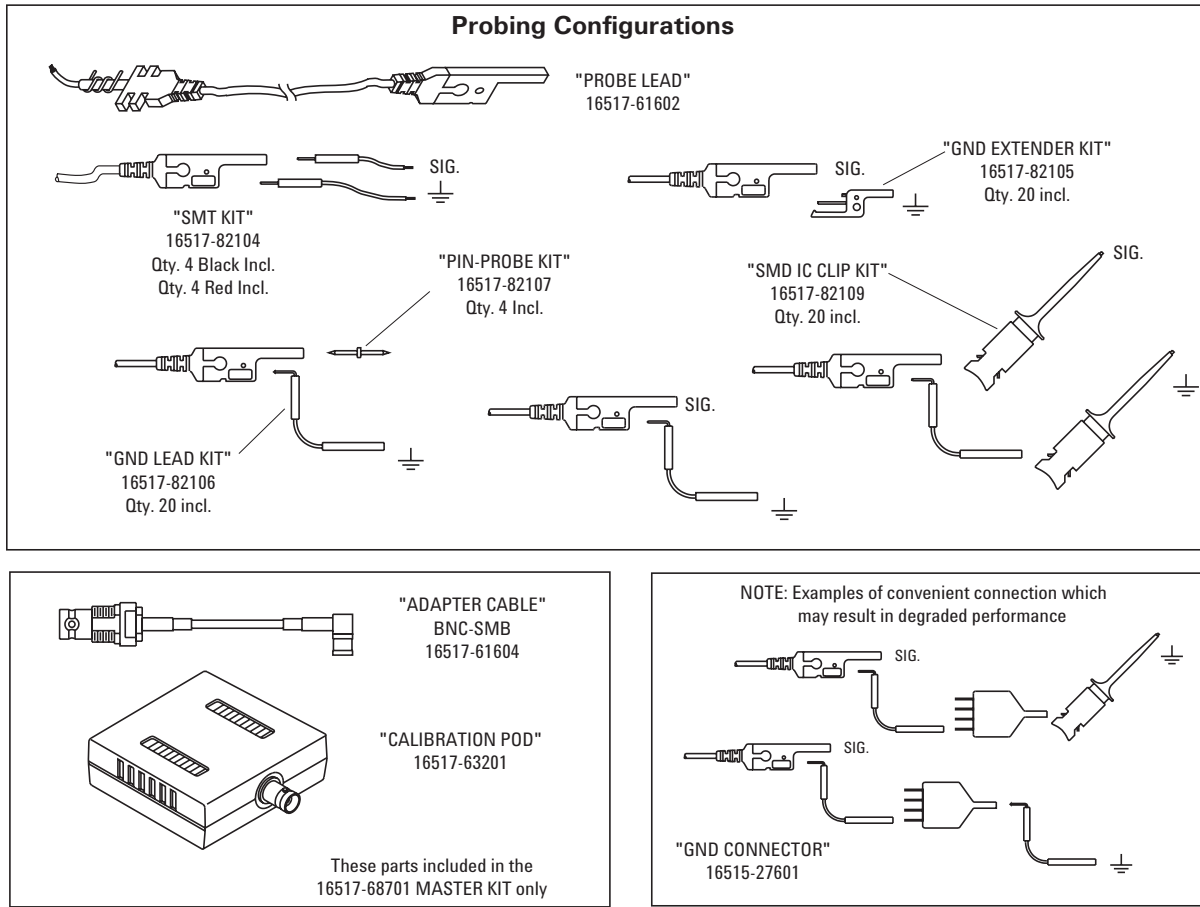


Figure 12.5. Agilent Technologies 16517-68701 master accessory kit and 16518-68701 expansion accessory kit

Recommended Probe Configurations

For the best performance, use the following configurations. The configurations are listed in the recommended order.

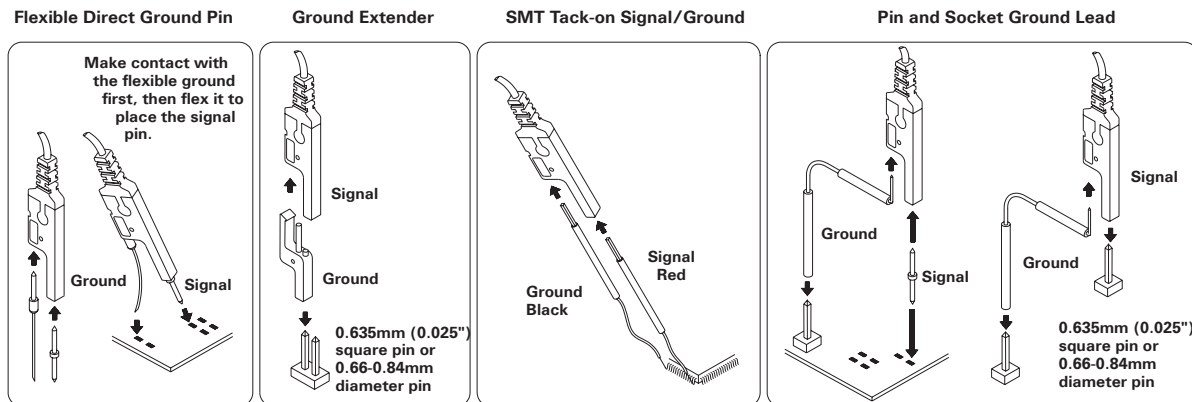


Figure 12.6. Probing configurations that give the best signal fidelity